



Well Dental Laboratory Co. Ltd.

Unit B, 2/F, Mackenny Centre, 660 Castle Peak Road
Lai Chi Kok, Kowloon, Hong Kong

Tel: 852) 2850-4433 | **Whatsapp:** (852) 9287-3860 | cs@welldental.com.hk

SCREW-RETAINED IMPLANT RESTORATIONS:

- Full Zirconia w/ Ti Base
- Porc. Fused to Zirconia/Ti Base
- Porc. Fused to Metal (CrCo)
- Dynamic® Abutment
w/ Angulated Screw Channel
- NobelProcera® Abutment
w/ Angulated Screw Channel
- Temporary Crown/Bridge

IMPLANT SUPPORT BRIDGE:

- Full Zirconia w/ Ti Framework
- Porc. Fused to Zirconia
w/ Ti Framework
- Porc. Fused to Metal (CrCo)

HYBRID:

- HK Bridge (Wire Reinforcement)
- Wrap Around (Ti Framework)

iWell® CAD/CAM CUSTOM IMPLANT ABUTMENTS

- Zirconia Abutment w/ Ti Base
- Titanium Abutment
 - Gold Anodized Coating
 - Pink Anodized Coating

iWell® CAD/CAM RESTORATIONS

- Crown
- Bridge
- Inlay
- Onlay
- Veneer
- Bonded Bridge

REMOVEABLE

- Full-Acrylic Denture
- Valplast® Flexible Denture
- Cast-Metal Partial Denture
- Locator
- Bar & Clip
- CAD/CAM Ti Bar

OTHERS

- CAD/CAM 3D Printed Models
- Mounted Models on Articulator
- Diagnostic Wax-Up
- Implant Surgical Guide
- Teeth Whitening Custom Tray
- Soft Night Guard
- Hard Night Guard
- Playsafe® Sportsguard

CHOOSE MATERIAL

- iWell® Monolithic Zirconia
- iWell® Multi-layer Zirconia
- 3M Lava® Plus
- 3M Lava® Esthetic
- NobelProcera® Zirconia

- IPS e.Max® Press Monolithic
w/ Stain
- IPS e.Max® Press Cut-Back
 - High Trans
 - Low Trans
 - Medium Opacity
 - Other: _____

- Full Cast Metal
- Porc. Fused to Metal
- Yellow Gold
- White Gold
- Chrome Cobalt

TEMPORARIES:

- Multi-layer PMMA
- PMMA
- Resin Composite

DOCTOR NAME:

PATIENT NAME:

FINAL SHADE:

STUMP SHADE:

Match Pictures

eLab® Shade Matching

INSTRUCTIONS:

CLINIC NAME/ADDRESS (Stamp):



DELIVERY BY:

Before 1pm

After 2pm



(Circle Teeth To Be Restored)

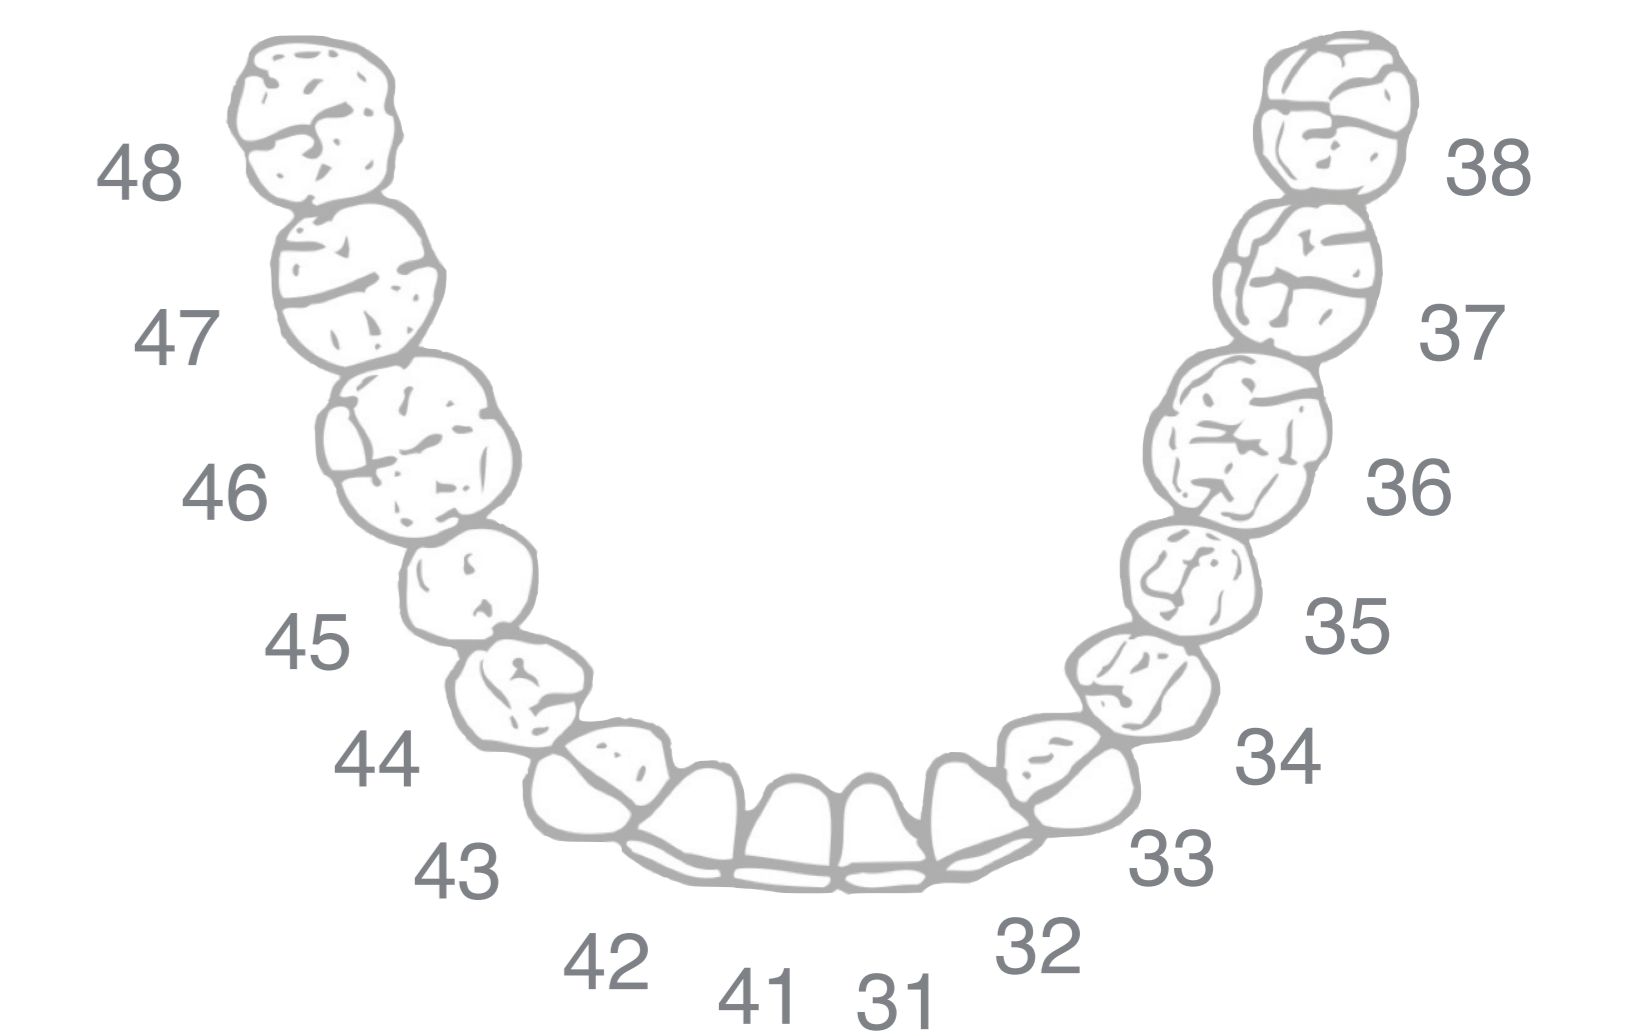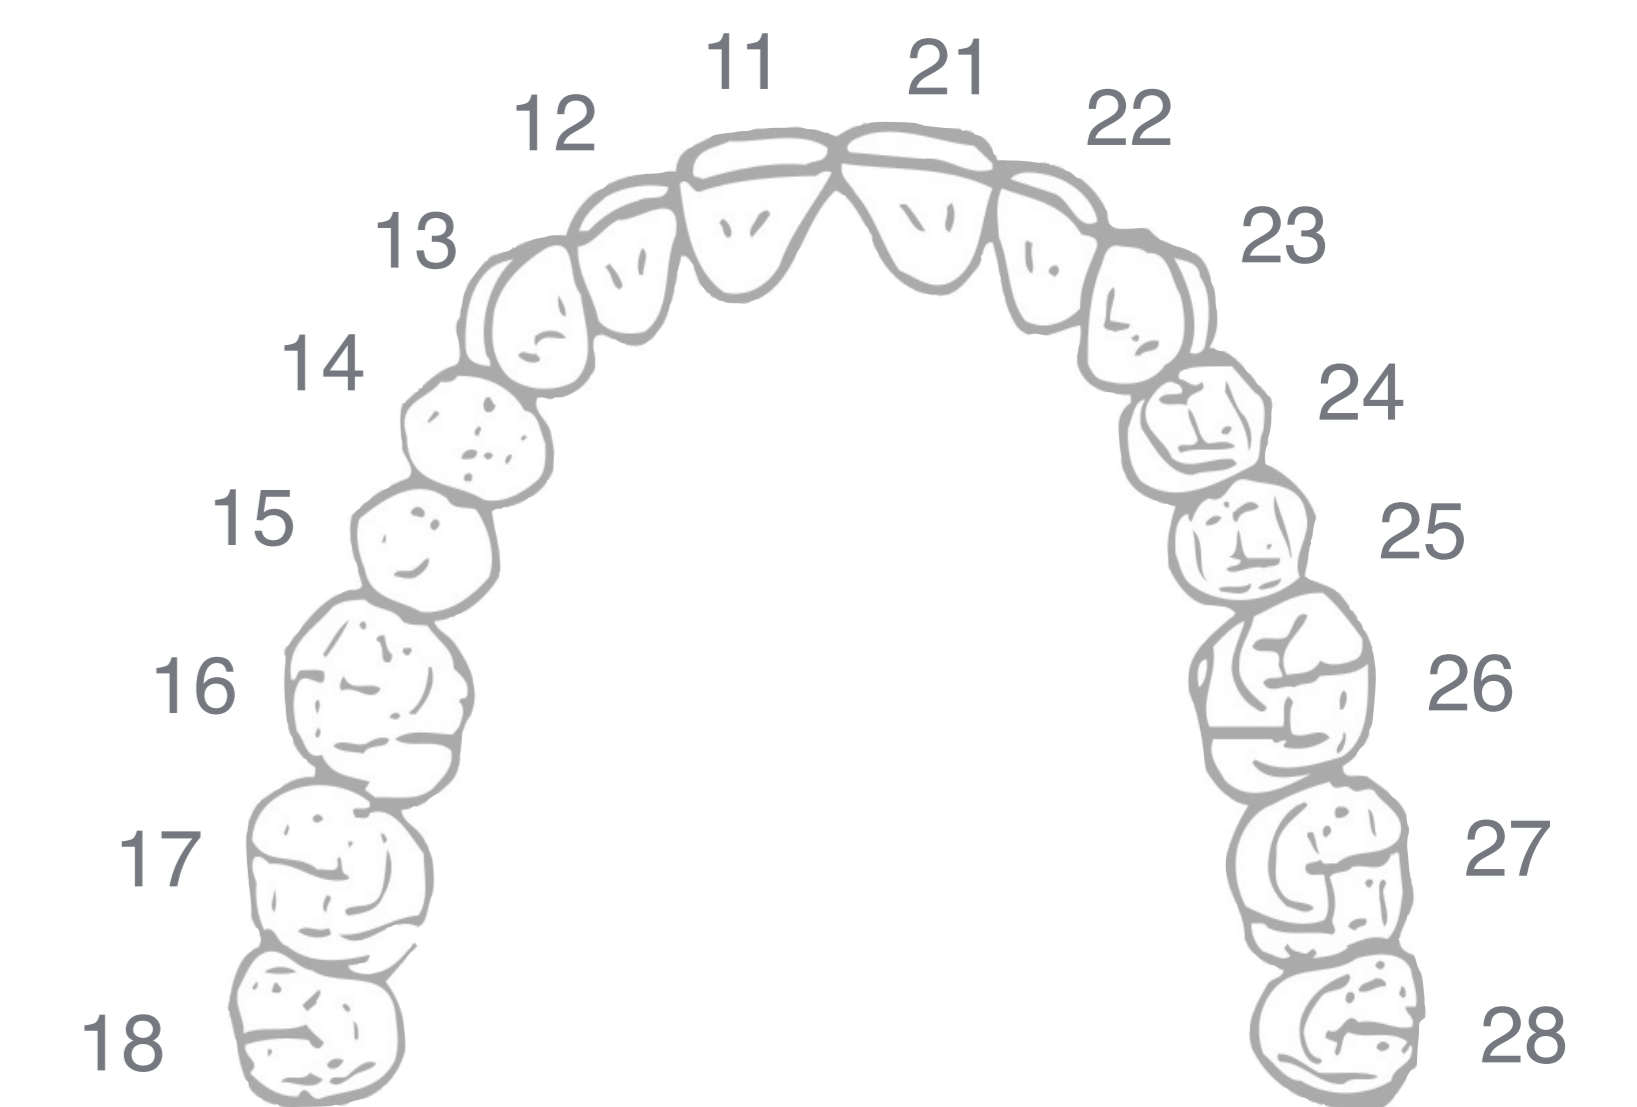


SIGNATURE: _____

RX DATE: _____

PONTIC DESIGN




CERAMIC MARGIN DESIGN

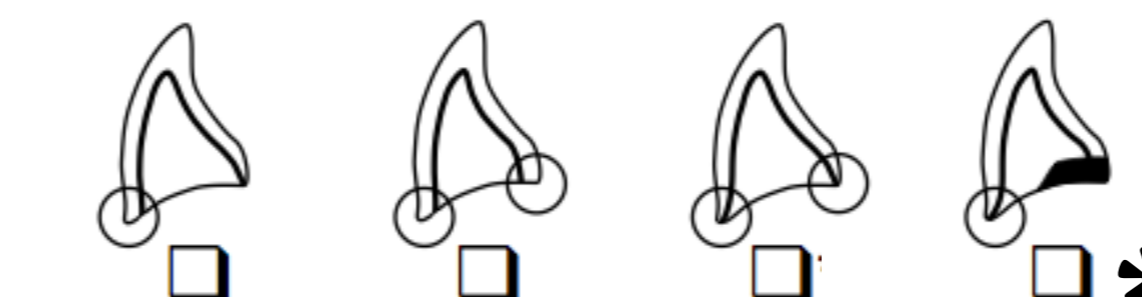

Labial Butt 360° Butt Junction Junction*

CERAMIC METAL DESIGN

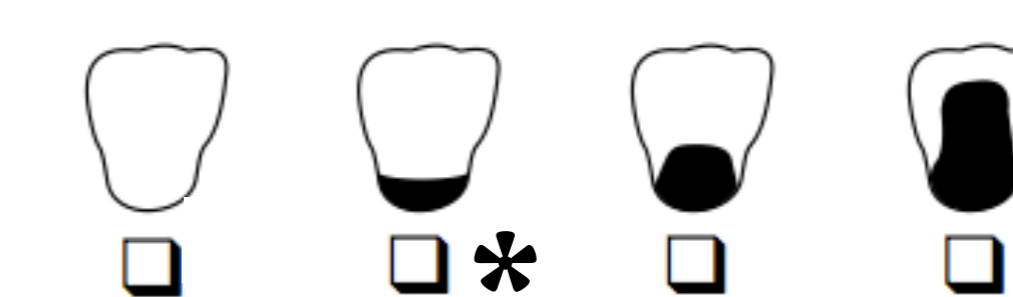

* Default parameters used unless specified

OCCLUSAL STAINING

None Light * Med Dark

CONTACTS

Point Normal * Broad

EMBRASURES

Closed * Open